

# NHS Sustainability: From Hero to Net Zero

Julia A. Meister

## Healthcare climate impact



Hospitals are the world's **5<sup>th</sup> worst polluter**.



The NHS produces **590,000t of waste**, costing **£700m annually**.



**Single-use medical devices** contribute the most waste.




### What is the goal?

To reduce single-use devices and their climate impact.



### What are the benefits?

Reinvesting saved waste processing funds.



### Why is it difficult?


There is no one-size-fits-all solution for sustainable medical devices.

## How to reduce single-use devices?

### Remanufacturing

- It **"resets"** tools as if they were **new** for safe reuse.
- It is **everywhere!** Take a kitchen knife:
  - Sharpen
  - Use
  - Wash
- Carefully regulated, this works for **single-use medical devices** too.

Remanufacturing may use a lot of resources too!

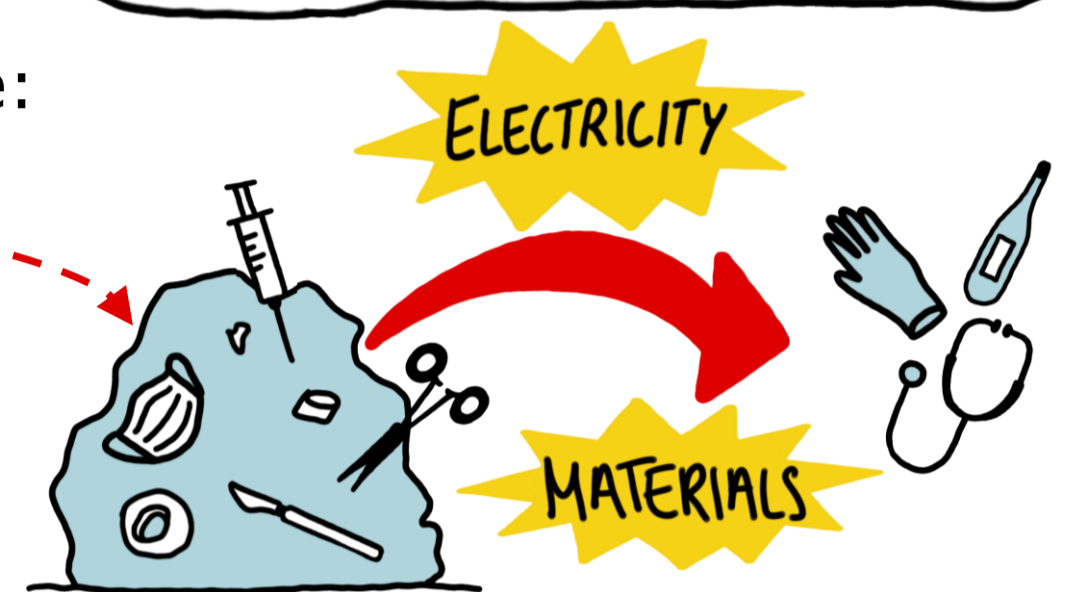

## Is remanufacturing **always** more sustainable?

## Custom emissions framework



Measuring **custom carbon emissions** is critical, so that **on-paper results reflect real impacts**.

Therefore, we customise device carbon footprints by:


- Modelling every life cycle in/output to calculate **realistic emissions** (Life Cycle Analysis).
- Identifying **impactful life cycle parameters** (Sensitivity Analysis).
- Future-proofing results by integrating **long-term use statistics** (Value Chain Analysis).

### Single-use device life cycle

#### Linear economy

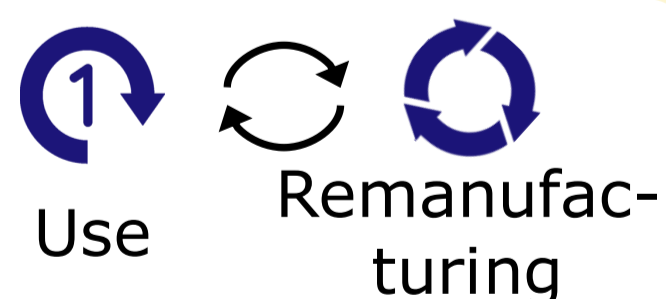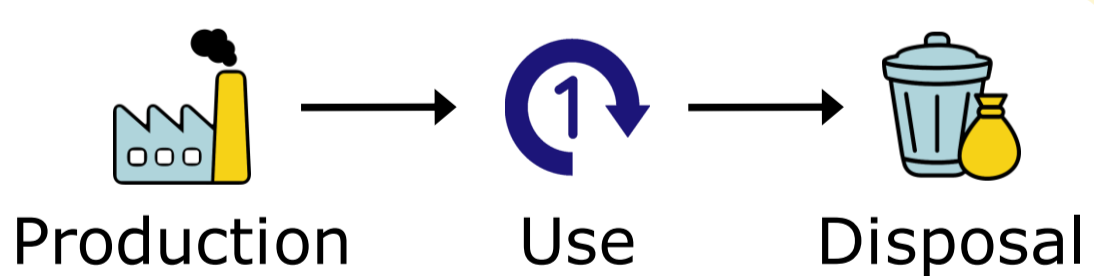

#### Circular economy

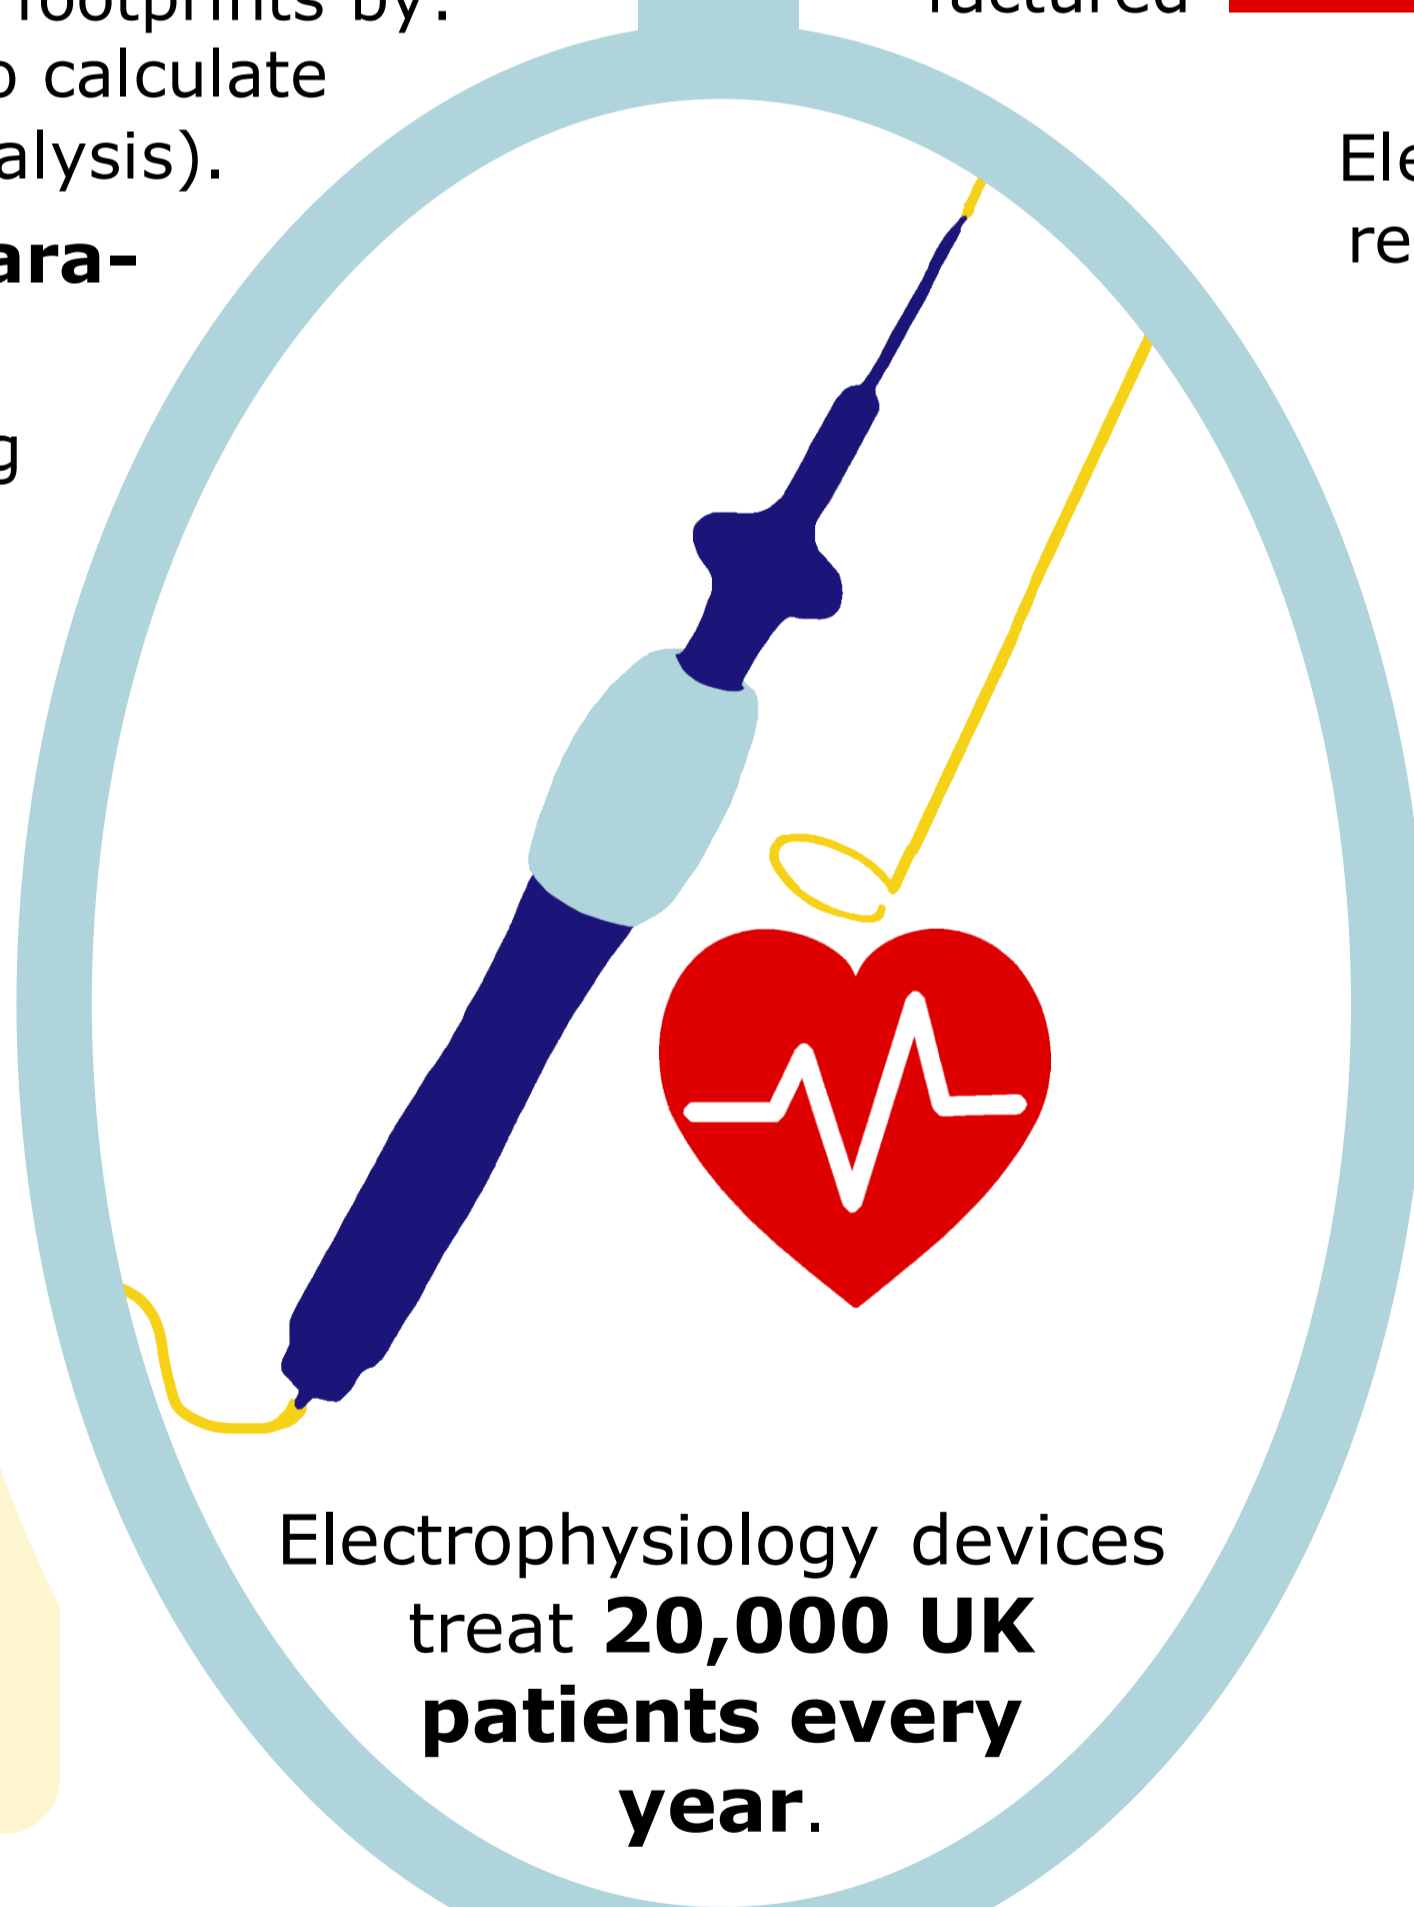

Electrophysiology devices treat **20,000 UK patients every year**.

## Sustainable procurement case study

### UK electrophysiology devices cost (per year)

New	<b>£5.3 million</b>
Remanufactured	<b>£2.9 million</b> <span style="color: red;">-45%</span>

Electrophysiology devices surgically restore **healthy heart rhythms**.




Most are **discarded after one use** – even though they are **safe to remanufacture**.



We explored **3 alternatives** to reduce NHS emissions (varying location, transport, resources).



### Electrophysiology device sustainability (per year)

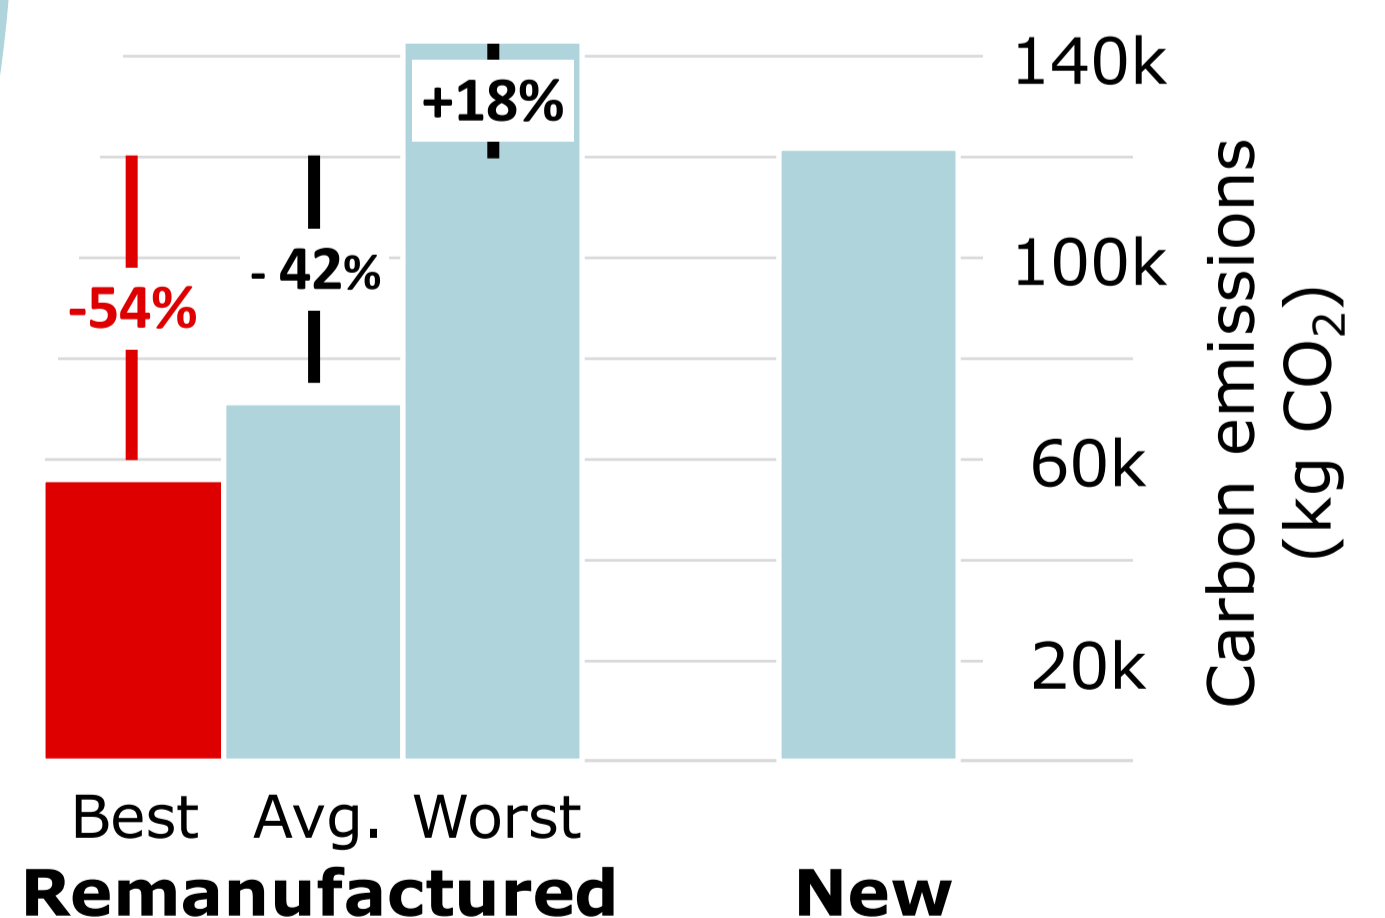

### How many new devices $C$ are needed?

$$U = \sum_{n=0}^N C \times (1 - R)^n$$

$U$ : Nr. total device uses  
 $C$ : Nr. new devices  
 $R$ : Rejection rate

### What are a hospital's device emissions?

$$Emissions_{total} = C \times Emissions_{new} + (U - C) \times Emissions_{reman}$$

$C \times Emissions_{new}$ : New device emissions  
 $(U - C) \times Emissions_{reman}$ : Remanufactured emissions

Up to **66,000kg CO<sub>2</sub> saved annually** with the **most sustainable** remanufactured electrophysiology devices.

Personalised emissions **empower hospitals** to find their **most sustainable** device **alternatives**.

**"Remove if you must, remanufacture if you may."**